
DL FLOWER | INSTRUCTION MANUAL

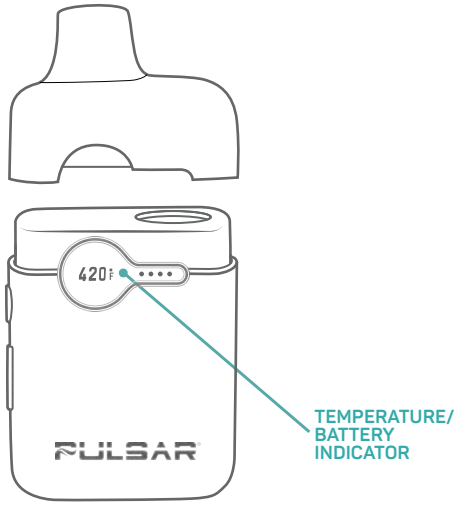

SPECS
Size: 3.5 x 1.9 x 1" (88 x 49 x 25.5 mm)
Chamber Size: 0.25 g
Battery Capacity: 1200 mAh
Temperature Range: 320 - 430°F (160 - 221°C)
Charging: USB-C

KIT INCLUDES
1x DL Flower
1x USB-C Charging Cable
1x Cleaning Brush
2x Mouthpiece Screens

CHARGING
Before using the DL Flower, fully charge the device using the USB-C charging cable and a standard charging brick. You will see the battery indicator lights flash when the battery is charging, and the battery indicator lights will represent the battery level. When the battery reaches 100%, the device is fully charged, and battery indicator lights will turn off. The device does not have pass-through functionality.

BATTERY INDICATOR
4 lights 75 - 100%
3 lights 50 - 75%
2 lights 25 - 50%
1 light 0 - 25% (Charge)

LOADING THE CHAMBER
With the device off, remove the mouthpiece. Fill the chamber to the top with finely ground material. It should fill the chamber completely, but not be packed too tightly. Depending on your material, 0.25 g should be enough. Replace the mouthpiece once the chamber is packed.

POWER ON/OFF
To power the device on or off, quickly press the button 5 times. The device will vibrate to let you know it is turning on or off. It will automatically start heating once it has been turned on.

TEMPERATURE SELECTION
The DL Flower has a temperature range of 320 to 430°F (160 - 221°C). Use the up and down buttons to select your preferred temperature in increments of 5 degrees. Once your preferred temperature is selected, the device will vibrate once it has hit that temperature. You can increase or decrease the temperature at any time during the session. The device will vibrate again to let you know the new temperature has been reached. You can convert the temperature read out to Celsius by holding the power button and the down button at the same time for 2 seconds.

VAPING SESSION TIMER
To adjust the session duration, hold down the power button for 2 seconds once the device is on. You can then adjust the session duration at any time between 3 minutes (180 seconds) to 5 minutes (300 seconds) in increments of 30 seconds. The display will only show the number of seconds for the session, please refer to the chart below for minutes.

180 - 3 minutes
210 - 3:30 minutes
240 - 4 minutes
270 - 4:30 minutes
300 - 5 minutes

DL FLOWER | INSTRUCTION MANUAL

VAPING

Once the device hits the selected temperature it will vibrate to let you know it is ready. At this point you can begin vaping. We recommend taking longer slower pulls to get the most out of the experience. Once you have finished the session, use the included stir tool to stir the material or discard it once it has been fully used. At the end of each session a count down timer will appear when there are 20 seconds left in the session. You can cancel the session at any time by pressing the power button 5 times and turning the device off.

CLEANING


To clean the main body and chamber, first remove the mouthpiece and set it aside. Next, you use the included cleaning brush to remove any build up in the chamber or surrounding area.

To disassemble the mouthpiece, start by firmly pressing against the mouthpiece so that it passes through the outer shell. Once the silicone housing has been removed, then remove the ceramic air path from the side of the housing. Finally, remove the silicone screen from the bottom of the housing, then use the cleaning brush to remove larger build up before soaking the pieces in alcohol for at least 30 minutes or until the build up is no longer there. Please allow all mouthpiece parts to fully dry before reassembly.

WARNINGS

Do not expose to extreme temperatures or direct sunlight. Do not drop the device or accessories. Do not drop or submerge in any liquid. Do not modify the electronics in any way. This device is intended for adults only. Do not sell or provide to minors. Keep all parts, concentrates, herbs, and liquids away from children and pets. This is not a medical device and is not intended to diagnose, treat, mitigate, cure, or prevent any ailment, disease, or other conditions. Consult a physician before use, especially if you suffer from heart disease or any other medical condition, or if you are pregnant or breastfeeding. Failure to follow any of these instructions could result in product damage, property damage, personal injury, and may void warranty. Visit PulsarShop.com for warranty information.

DL FLOWER | INSTRUCTION MANUEL

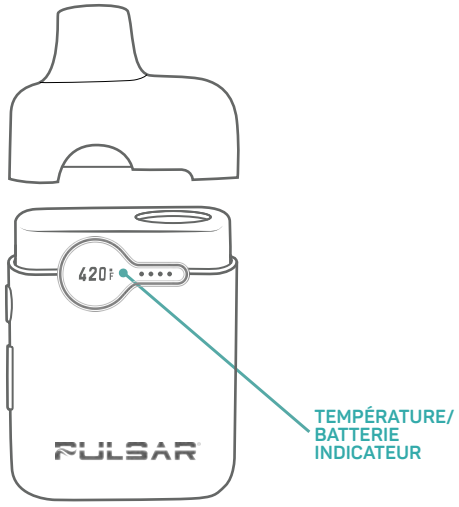

CARACTÉRISTIQUES
Dimensions: 88 x 49 x 25,5 mm (3,5 x 1,9 x 1 po)
Taille de la chambre: 0,25 g
Capacité de la batterie: 1200 mAh
Plage de température: 160 - 221°C (320 - 430°F)
Chargement: USB-C

LE KIT COMPREND
1x Fleur DL
1x Câble de Chargement USB-C
1x Brosse de Nettoyage
2x Écrans d'embout Buccal

CHARGEMENT
Avant d'utiliser le DL Flower, chargez complètement l'appareil à l'aide du câble de chargement USB-C et d'une brique de chargement standard. Les voyants de batterie clignotent pendant la charge et indiquent le niveau de charge. Lorsque la batterie atteint 100%, l'appareil est complètement chargé et les voyants s'éteignent. L'appareil ne dispose pas de fonction de transfert.

INDICATEUR DE BATTERIE
4 lumières 75 - 100%
3 lumières 50 - 75%
2 lumières 25 - 50%
1 lumière 0 - 25% (Charge)

CHARGEMENT DE LA CHAMBRE
L'appareil étant éteint, retirez l'embout buccal. Remplissez la chambre jusqu'en haut avec du matériau finement moulu. La quantité doit être entièrement remplie, sans être trop compacte. Selon le matériau, 0,25 g devrait suffire. Remettez l'embout buccal une fois la chambre remplie.

MARCHE/ARRÊT
Pour allumer ou éteindre l'appareil, appuyez rapidement 5 fois sur le bouton. L'appareil vibrera pour vous indiquer qu'il s'allume ou s'éteint. Il commencera automatiquement à chauffer une fois allumé.

SÉLECTION DE LA TEMPÉRATURE
Le DL Flower offre une plage de température de 160 à 221 °C (320 à 430 °F). Utilisez les boutons haut et bas pour sélectionner la température souhaitée par incréments de 5 degrés. Une fois la température sélectionnée, l'appareil vibre dès qu'il l'atteint. Vous pouvez augmenter ou diminuer la température à tout moment pendant la séance. L'appareil vibre à nouveau pour vous indiquer que la nouvelle température est atteinte. Vous pouvez convertir la température affichée en degrés Celsius en maintenant simultanément les boutons marche/arrêt et bas pendant 2 secondes.

MINUTERIE DE SÉANCE DE VAPOTAGE
Pour régler la durée de la session, maintenez le bouton d'alimentation enfoncé pendant 2 secondes une fois l'appareil allumé. Vous pouvez ensuite la régler à tout moment, de 3 minutes (180 secondes) à 5 minutes (300 secondes), par incréments de 30 secondes. L'écran affichera uniquement le nombre de secondes de la session ; veuillez consulter le tableau ci-dessous pour connaître les minutes.

180 - 3 minutes
210 - 3:30 minutes
240 - 4 minutes
270 - 4:30 minutes
300 - 5 minutes

DL FLOWER | INSTRUCTION MANUEL

VAPOTAGE

Une fois la température sélectionnée atteinte, l'appareil vibre pour vous indiquer qu'il est prêt. Vous pouvez alors commencer à vapoter. Nous vous recommandons de vapoter plus lentement et plus longtemps pour une expérience optimale. Une fois la session terminée, utilisez le mélangeur fourni pour remuer le contenu ou jetez-le une fois utilisé. À la fin de chaque session, un compte à rebours apparaît lorsqu'il reste 20 secondes de vapotage. Vous pouvez annuler la session à tout moment en appuyant 5 fois sur le bouton d'alimentation et en éteignant l'appareil.

NETTOYAGE

Pour nettoyer le corps principal et la chambre, retirez d'abord l'embout buccal et mettez-le de côté. Utilisez ensuite la brosse de nettoyage fournie pour éliminer toute accumulation dans la chambre ou autour.

Pour démonter l'embout buccal, appuyez fermement dessus pour le faire passer à travers la coque extérieure. Une fois le boîtier en silicone retiré, retirez le conduit d'air en céramique situé sur le côté du boîtier. Enfin, retirez l'écran en silicone du dessous du boîtier, puis utilisez la brosse de nettoyage pour éliminer les dépôts les plus importants avant de tremper les pièces dans de l'alcool pendant au moins 30 minutes ou jusqu'à ce que les dépôts disparaissent. Laissez sécher complètement toutes les pièces de l'embout buccal avant de les remonter.

AVERTISSEMENTS

Ne pas exposer à des températures extrêmes ni à la lumière directe du soleil. Ne laissez pas tomber l'appareil ni ses accessoires. Ne le laissez pas tomber ni ne l'immergez dans un liquide. Ne modifiez en aucune façon les composants électroniques. Cet appareil est destiné aux adultes uniquement. Ne pas vendre ni fournir aux mineurs. Tenez toutes les pièces, concentrés, plantes et liquides hors de portée des enfants et des animaux. Ceci n'est pas un dispositif médical et n'est pas destiné à diagnostiquer, traiter, atténuer, guérir ou prévenir une quelconque maladie ou affection. Consultez un médecin avant utilisation, surtout si vous souffrez d'une maladie cardiaque ou de tout autre problème médical, ou si vous êtes enceinte ou allaitez. Ne pas respecter ces instructions peut entraîner des dommages au produit, des dommages matériels, des blessures corporelles et l'annulation de la garantie. Consultez PulsarShop.com pour plus d'informations sur l'autorisation.