
DABTRON 2 | INSTRUCTION MANUAL

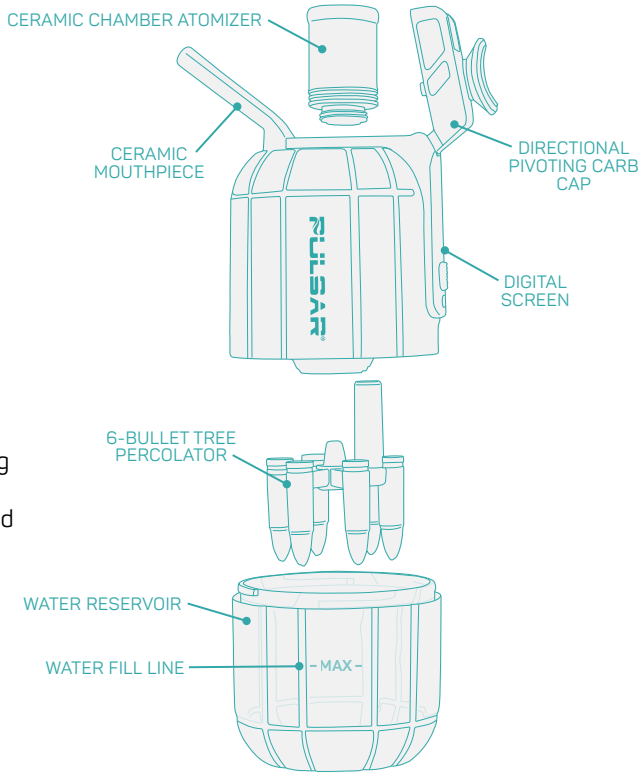

SPECS
Size: 2.43 x 2.34 x 5.04" (61.7 x 59.5 x 128 mm)
Battery: 1500 mAh
Temp setting: 400, 450, 500, 550°F (204 – 288°C)
Charging: USB-C

KIT INCLUDES
1x Pulsar Dabtron 2.0
1x USB-C Charging Cable
5x Extended Alcohol Swabs
5x Cotton Swabs

CHARGING
Before using the Dabtron 2.0, fully charge the device using the USB-C charging cable and a standard charging brick. Charging will be indicated by the pulsating battery icon and the LED light in the base will flash Red. When the device is fully charged, the battery icon will be full and the light will turn off. Do not use fast charging adapters. Please use only the original charging cable included in the package.

1 Bar: 0 – 25%
2 Bars: 25 – 50%
3 Bars: 50 – 75%
4 Bars: 75 – 100%

WATER FILTRATION
Twist the base a quarter turn, clockwise, to remove it from the device. Add water to the fill line before reattaching it to the device.

POWERING ON/OFF
Remove the charging cable from the device and press the power button 5 times to turn the device on or off. You will feel the device vibrate twice and the light that corresponds to the temperature setting will flash.

TEMPERATURE SELECTION
The Dabtron 2.0 is equipped with 4 preset temperatures. With the device on, you can cycle through the settings by pressing the power button 1 time. To select your setting, simply stop on the desired setting once it is highlighted Yellow. The device will vibrate to let you know the setting has changed.

Low: 400°F - Yellow Medium: 450°F - Green High: 500°F - Blue Turbo: 550°F - Red

LOADING CONCENTRATE
With the device powered on and your setting selected, flip open the atomizer cover to reveal the ceramic chamber atomizer. Place a small amount of concentrate in the atomizer and then close the atomizer cover.

USAGE
To begin, press the power button twice to start the preheat cycle. The device will vibrate once to confirm it is preheating. During preheat, the selected setting will be highlighted with a pulsating Blue light while the base lights cycle through different colors. The device will vibrate again when your session is ready to begin. The selected setting and base light will flash Green. The session will end after 40 seconds and the device will vibrate twice to let you know it has finished.

You can cancel the session at any time by pressing the power button 2 times.



PulsarShop.com

PU-0868-25

DABTRON2™ | INSTRUCTION MANUAL

COIL MAINTENANCE
For optimal performance, wipe out your ceramic chamber atomizer with a cotton swab after each session.

After multiple sessions, clean out any lingering buildup to keep the coil working as long as possible. Dip a cotton swab in isopropyl alcohol before wiping out the atomizer. Please be sure to let the atomizer cool down before cleaning, and wipe up any residual solvent left inside.

The coil can be soaked in alcohol for a deep cleaning. Let the coil soak for at least 30 minutes before removing it from the alcohol. Be sure to let the coil fully air dry before using it again. Never rinse with water.

PERCOLATOR MAINTENANCE
Caution - Clean the base with an alcohol solution under 75%. Do not immerse, may damage plastic. Twist the base clockwise to remove it from the Dabtron and discard the water. Next remove the percolator by pulling straight down away from the device. Use a cotton swab and the 75% alcohol solution to wipe off any build up from the base and percolator. Soak the percolator in the 75% alcohol solution for up to an hour to remove any build up inside.

When you remove the sticker from the device, it might leave some residue. 70-75% isopropyl alcohol will remove the sticker residue from the base.

AIR PATH AND ATOMIZER CONNECTION
To clean the airpath, use the included Extended Alcohol Swab to clean any buildup below the atomizer and below the mouthpiece. Use a regular cotton swab and 91% (or higher) isopropyl alcohol to clean the threading and connection.

MOUTHPIECE
Use the Extended Alcohol Swab to clean the mouthpiece.

TROUBLESHOOTING
No Connection: The light in the base will flash White 3 times, the screen will stay off.
Short Circuit and Overload Protection: The light in the base will flash Red 3 times, the screen will stay off.

WARNINGS
Do not expose to extreme temperatures or direct sunlight. Do not drop the device or accessories. Do not drop or submerge in any liquid. Do not modify the electronics in any way. This device is intended for adults only. Do not sell or provide to minors. Keep all parts, concentrates, herbs, and liquids away from children and pets. This is not a medical device and is not intended to diagnose, treat, mitigate, cure, or prevent any ailment, disease, or other conditions. Consult a physician before use, especially if you suffer from heart disease or any other medical condition, or if you are pregnant or breastfeeding. Failure to follow any of these instructions could result in product damage, property damage, personal injury, and may void warranty. Visit PulsarShop.com for warranty information.