

VOYAGER | INSTRUCTION MANUAL

SPECS
Size: 1.06 x 1.89 x 3.59" (27 x 48 x 91.3 mm)
Chamber Capacity: 0.3–0.4 g
Pod Capacity: 0.2–0.25 g
Battery Capacity: 2000 mAh
Temperature Range: 370, 390, 410, 430°F
Charging: USB-C

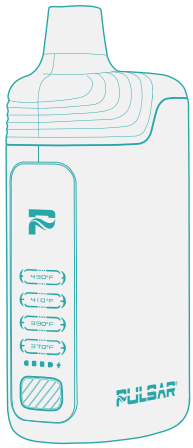

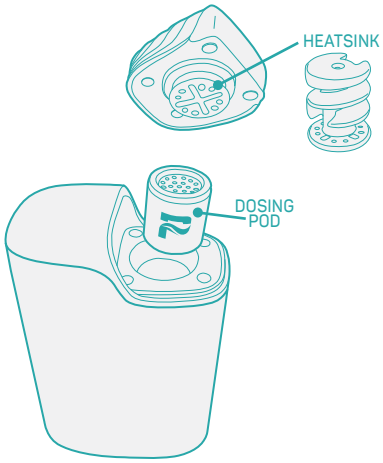

KIT INCLUDES
1x Pulsar Voyager
2x Dosing Pods
5x Extended Alcohol Swabs
1x USB-C Charging Cable

CHARGING
Before using the Voyager, fully charge the device using the USB-C charging cable and a standard charging brick. Once the cable is inserted, the device will vibrate to confirm the connection. The battery bars light up from left to right and a lightning bolt symbol flashes during charging. When all 4 battery bars are solid, the device is fully charged. The device does not have pass-through functionality. The battery bars will represent the battery level.

- 1 bar - 0–25%
- 2 bars - 25–50%
- 3 bars - 50–75%
- 4 bars - 75–100%

When the battery has been depleted, the lightning bolt symbol will flash and 1 bar will be displayed in red. A full recharge will take 110 minutes.

BEFORE USE
You can use the Voyager with or without a convenient dosing pod. One dosing pod comes preinstalled in the device. We recommend running 1 heat cycle with the pod unloaded in the chamber to remove any lingering manufacturing oils.

LOADING THE DOSING POD
Use the onboard stir tool to dislodge the dosing pod by inserting it all the way into the airflow intake hole on the bottom of the device. Remove the silicone lid from the pod and add around 0.25 g of finely ground material. It should fill the pod completely, but not be packed too tightly. Replace the lid on the dosing pod and slide the dosing pod back into the chamber. If the silicone lid accidentally is pushed too far into the pod, you can use the fine tip of the stir tool as a hook to pull the lid upward.

LOADING THE CHAMBER
If you choose to use the device without a dosing pod, follow these steps. With the device off, remove the mouthpiece. Fill the chamber to the top with around 0.35 g of finely ground material. It should fill the chamber completely, but not be packed too tightly. Replace the mouthpiece once the chamber is packed.

POWER ON/OFF
To power the device on or off, press and hold the button for 1.5 seconds. The device will vibrate to confirm.

TEMPERATURE SELECTION
With the device on, press the button 1 time to cycle to the next temperature. The device will always start from the last selected temperature.

370°F
390°F
410°F
430°F

PULSAR®

PulsarShop.com

PU-0951-26

VAPING

With the device loaded and the temperature selected, press the button 2 times quickly to start the preheat cycle. The device will vibrate 1 time and the selected temperature will flash during the preheat cycle. The device will vibrate 2 times and the selected temperature will remain solid to let you know it has reached the selected temperature and is ready for use. The heating cycle will last 3 minutes; you can end the session at any point by pressing the button 2 times. Inhale slowly from the mouthpiece to get the best experience. Once the session has ended, the device will vibrate 2 times and the screen will fade out.

NOTE: To keep the device from overheating, allow 10 minutes between sessions.

CLEARING THE DOSING POD/CHAMBER

Once the session has ended, allow the device to cool down before removing the onboard stir tool as it can become hot during use. Remove the dosing pod with the stir tool as described previously, then remove the silicone lid and clear the material from the dosing pod with the tool. If material is packed directly in the chamber, use the stir tool to clear the material. Clean the stir tool and replace it in the bottom of the device.

NOTE: The metal part of the stir tool will be hot immediately following a heat cycle. We recommend only handling the tool by the silicone base until it is cool to the touch.

CLEANING

To clean the mouthpiece, disassemble it by gently pulling out the ceramic heatsink. Soak both pieces in 91%+ isopropyl alcohol for 1 hour to remove any buildup. Be sure to replace the heatsink with the spiral end towards the chamber for proper airflow.

To clean the dosing pods, remove the lid and soak both pieces in 91%+ alcohol for 1 hour to remove any buildup.

To clean the chamber, use a cotton swab dipped in 91%+ alcohol to wipe away any buildup in the chamber.

Allow all parts to fully air dry before reassembly.

WARNINGS

Do not expose to extreme temperatures or direct sunlight. Do not drop the device or accessories. Do not drop or submerge in any liquid. Do not modify the electronics in any way. This device is intended for adults only. Do not sell or provide to minors. Keep all parts, concentrates, herbs, and liquids away from children and pets. This is not a medical device and is not intended to diagnose, treat, mitigate, cure, or prevent any ailment, disease, or other conditions. Consult a physician before use, especially if you suffer from heart disease or any other medical condition, or if you are pregnant or breastfeeding. Failure to follow any of these instructions could result in product damage, property damage, personal injury, and may void warranty. Visit PulsarShop.com for warranty information.